


# TruSeq Custom Amplicon Kit Dx<sup>®</sup>

## Workflow and Kit Tracking Form

FOR *IN VITRO* DIAGNOSTIC USE

For detailed instructions, refer to the *TruSeq Custom Amplicon Kit Dx Package Insert (document # 1000000029772)*.

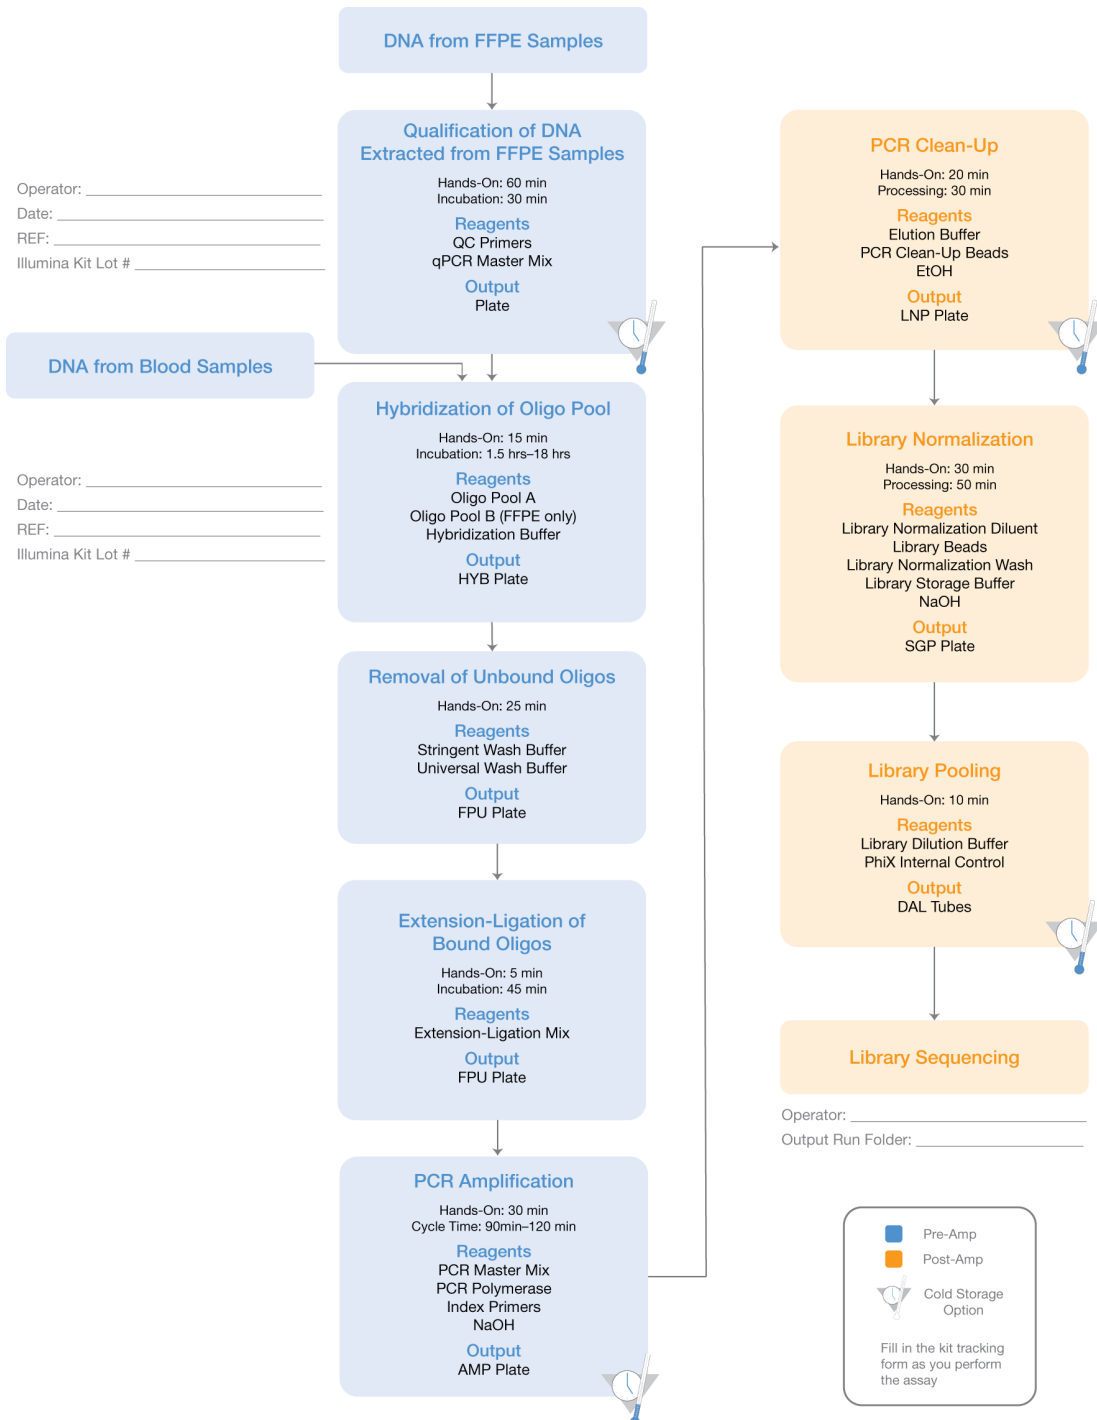


# TruSeq Custom Amplicon Kit Dx

## Workflow and Kit Tracking Form

[This page intentionally left blank]



Illumina  
5200 Illumina Way  
San Diego, California 92122 U.S.A.  
+1.800.809.ILMN (4566)  
+1.858.202.4566 (outside North America)  
techsupport@illumina.com  
[www.illumina.com](http://www.illumina.com)



Illumina Netherlands B.V.  
Steenoven 19  
5626 DK Eindhoven  
The Netherlands



Australian Sponsor:  
Illumina Australia Pty Ltd  
Nursing Association Building  
Level 3, 535 Elizabeth Street  
Melbourne, VIC 3000  
Australia